



Instrument: MSD 20
 Mon Jul 24 11:14:38 2006

D:\MSDCHEM\1\5973N\ATUNE.U

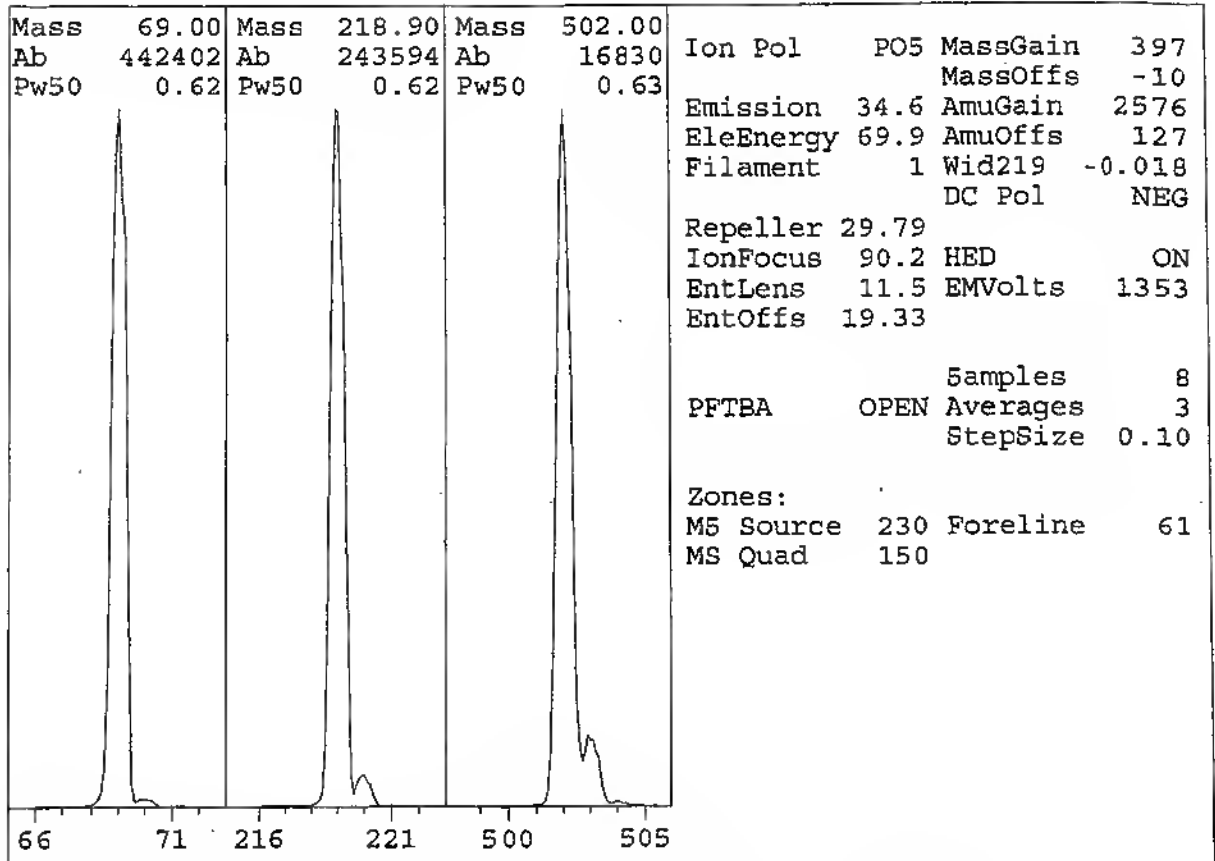

Scan: 10.00 - 700.00 Samples: 8 Thresh: 100 Step: 0.10
 127 peaks Base: 69.00 Abundance: 397824

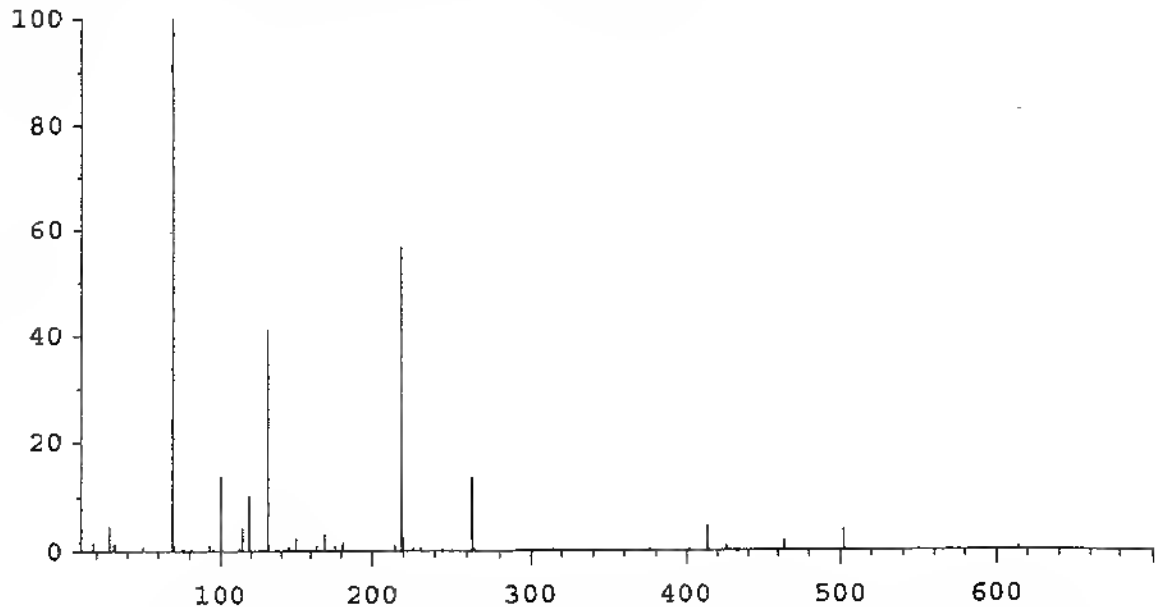

Mass	Abund	Rel Abund	Iso Mass	Iso Abund	Iso Ratio
69.00	397824	100.00	70.00	4362	1.10
219.00	225088	56.58	220.00	9995	4.44
502.00	15492	3.89	503.00	1554	10.03